

OWNER'S MANUAL



Mighty Bariatric Wheelchair



Thank you for purchasing this Mighty Bariatric Wheelchair. It is strongly recommended that you read through this user manual prior to using your Mighty Bariatric Wheelchair for the first time. Your Mighty Bariatric Wheelchair should provide years of trouble-free use, provided that you adhere to these recommendations.

WE ARE HERE TO HELP YOU

To request product service and order replacement parts, please call:

Customer Service: 07 3355 8000

Spare Parts: 07 3355 8007

8.30 am to 5.00 pm Monday to Friday

Email: sales@evocare.com.au

If the product does not function properly contact **Evocare Australia.**

When requesting service, please provide the following information:

1. Part Code and Description
2. Date of Purchase

Address: Evocare Australia Pty Limited
260 South Pine Road, Enoggera, Qld. 4051
P.O. Box 1144, Stafford, Qld. 4053

DESCRIPTION

Mighty Bariatric Wheelchair

Removable padded
desk length armrests

Nylon upholstery

Seat width
71cm (28") W x 50cm (20") D

Net Weight 46kgs

Double Cross Bar,
black colour

Height
adjustable with
triple axle
design



Grey hammertone
finish

Padded elevating leg rests
with security stainless steel
ratchet bar lock system

Aluminium foot plates

Option: Padded Seat Cushion—LM9808C

Note: Maximum user weight for this wheelchair is **318kgs**

Evocare is a quality endorsed company and supplies equipment listed with the Therapeutic Goods Administration.

The ARTG number for the **LM9808** Mighty Bariatric Wheelchair is **218602**.

DESCRIPTION

Mighty Bariatric Wheelchair

Double Cross Bar, black colour



Height adjustable with triple axle design



Removable padded desk length armrests



Parking Brake Lever



Elevating leg rests with security stainless steel ratchet bar lock system

Adjustable Padded Calf Pad

Aluminium foot plates



SPARE PARTS

Evocare Code

Description

Spare Parts for (LM9808)

9SK1U8081	Seat Nylon width 28"W x 20" D
9SK1U8082	Back Nylon with embroidery 28" WIDE
9SK1A8081L	Armrest pads and screws. Restaurant style. - LH
9SK1A8081R	Armrest pads and screws. Restaurant style. - RH
9SK1W8081	Front wheel including bearing (each)
9SK1W8082	Bearings for front castors (each)
9SK1L8081L	Foot plates - LH
9SK1L8081R	Foot plates - RH



The comfort convoluted (egg shell) foam cushion – LM9808C is an option


MODIFICATION

Making LM9808 Wheelchair Non-Folding

In hospitals and nursing homes, theft of wheelchairs is often a common problem. Because most wheelchairs can be folded, they can easily be placed into the boot of a vehicle. These losses causes expense and inconvenience to institutions that rely on wheelchairs for the safe transport of people. Theft is less likely with a non-folding wheelchair.



Rivet positions for LM9808 Wheelchair

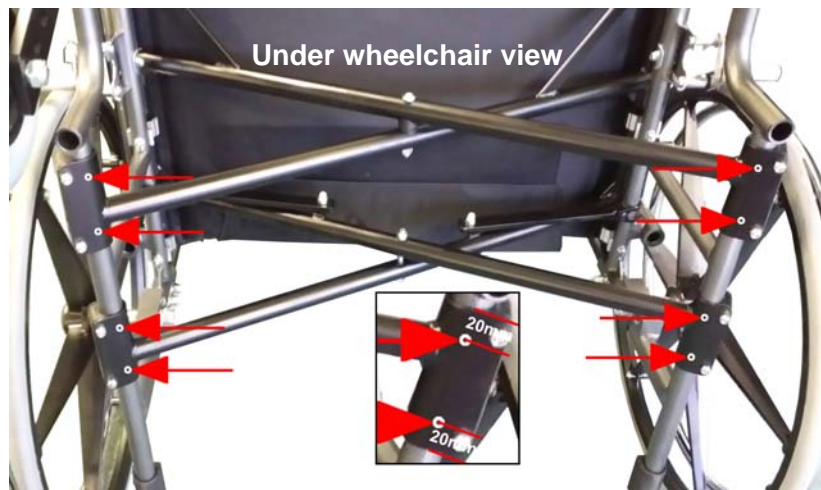

Procedure:

- .Ensure wheelchair is fully unfolded—At its full width.
- .Use 8 x 3/16” Stainless Steel Rivets.
- .Place rivets 20mm from each end of the bracket and in the middle of the bracket
- .Use 1/8” drill bit for initial holes then use 3/16” drill bit to finish hole to correct size.
- .A pneumatic rivet tool is best, although a hand lever type may be used—it will be difficult with a standard rivet tool, as rivets are large and stainless steel—NOTE: Only use stainless steel rivets.
- .One location on each side should be drilled and riveted before other holes are drilled so holes don't become misaligned.

Advantages:

- .Easier to propel and turn due to the frame rigidity—No energy lost in frame movement.
- .Greater strength and durability; parts moving less.
- .Less likely to be stolen as it is harder to transport.

A Comfort Cushion (LM9808C) is recommended as there will be less give in the seat. 6

OPTIONAL

IV Pole, Oxygen Bottle Holder Attachment

A two-prong, chrome plated steel IV with telescoping stem which can be easily height adjusted, allowing use of medication while on the move

With attached chrome plated steel oxygen bottle holder is designed to fit a "C" size cylinder. Perfect for people who need to bring their Oxygen cylinder with them.

Product Code: **9SK1H0005**



Attaches at handle



Attaches at axle

Safety / Handling of Bariatric Wheelchairs

Safety and handling of the Bariatric wheelchair requires the close attention of the Bariatric wheelchair user as well as the assistant. This manual points out the most common procedures and techniques involved in the safe operation and maintenance of the Mighty Bariatric wheelchair. It is important to practice and master these safe techniques until you are comfortable in manoeuvring around the frequently encountered architectural barriers.

Use this information only as a basic guide. The techniques that are discussed on the following pages have been used successfully by many users.

Individual Bariatric wheelchair users often develop skills to deal with daily living activities that may differ from those described in this manual. All warnings and cautions given in this manual **MUST** be followed.

Techniques in this manual are a starting point for the new Bariatric wheelchair user and assistant with safety as the most important consideration for all.

Stability and Balance

To assure stability and proper operation of your Mighty Bariatric wheelchair, you must at all times maintain proper balance. Your Mighty Bariatric wheelchair has been designed to remain upright and stable during normal daily activities as long as you do not move beyond the centre of gravity.

Virtually all activities which involve movement in the Mighty Bariatric wheelchair have an effect on the centre of gravity. Use the adjustable seatbelt for additional safety.

DO NOT lean forward out of the Mighty Bariatric wheelchair any further than the length of the armrests. Make sure the castors are pointing in the forward position whenever you lean forward. This can be achieved by advancing the Mighty Bariatric wheelchair and then reversing a little in a straight line.

Operating Instructions

To determine and establish your particular safety limits, practice bending, reaching and transferring activities in several combinations in the presence of a qualified health professional before attempting active use of the Mighty Bariatric wheelchair.

ALWAYS check hand grips for looseness before using the Mighty Bariatric wheelchair. If loose and/or worn, replace immediately.

If the Mighty Bariatric wheelchair is exposed to extreme temperature (above 38°C or below 0°C), high humidity and/or becomes wet, prior to use, ensure hand grips DO NOT twist on the Mighty Bariatric wheelchair handle—otherwise damage or injury may occur.

DO NOT attempt to reach objects if you have to move forward in the seat as this may tip the wheelchair.

DO NOT attempt to reach objects if you have to pick them up from the floor by reaching down between your knees as this may tip the wheelchair.

DO NOT lean over the top of the back upholstery to reach objects behind you, as this may tip the wheelchair.

DO NOT shift your weight or sitting position toward the direction you are reaching, as this may tip the wheelchair.

DO NOT tilt the Mighty Bariatric wheelchair without assistance.

DO NOT use an escalator to move a wheelchair between floors—serious injury may occur.

NEVER leave an unoccupied Mighty Bariatric wheelchair on an incline.

DO NOT attempt to stop a moving Mighty Bariatric wheelchair with the wheel locks. Wheel locks are not brakes.

Before attempting to transfer in or out of the Mighty Bariatric wheelchair, every precaution should be taken to reduce the gap distance. Turn both castors parallel to the object you are transferring onto. When transferring to and from the Mighty Bariatric wheelchair, ALWAYS lock both hand brakes (locks) before transferring to and from the Mighty Bariatric wheelchair.

DO NOT sit or transfer into the Mighty Bariatric wheelchair unless it is fully open.

DO NOT operate on roads, streets or highways.

DO NOT climb, go up or down ramps or traverse slopes greater than 9°.

DO NOT attempt to move up or down an incline which has a film of water, ice or oil on it.

DO NOT attempt to ride over kerbs or obstacles. Doing so may cause your Mighty Bariatric wheelchair to tip, causing bodily harm or damage to the wheelchair.

DO NOT over tighten hardware attaching to the frame. This could cause damage to the frame tubing.

Quick Release Components

The Mighty Bariatric wheelchair comes with a number of components which can be easily removed without tools for storage or transport.

Armrests

Remove the armrest by pushing in the button on the armrest tubing (1) whilst lifting the armrest up (2).

Because the armrest are detachable , DO NOT lift the wheelchair by the armrests.

Using the Stepper Tube

Use the stepper tube to raise the front castors (when mounting a low kerb for example). To use, push down on the stepper tube with your foot. DO NOT raise the front castors by pushing down on the push handles as this could tip the wheelchair.

To mount a low kerb. Approach the low kerb head on. Then the assistant uses the stepper tube to raise the front castors, and lowers the front castors on the raised kerb. Finally the assistant should push the wheelchair forward, lifting it up slightly to mount the kerb if required.


To go down a low kerb. Line up the front castors with the edge of the low kerb. The assistant uses the stepper tube to raise the front castors and tip the users back slightly. Keeping the castors raised slowly move the wheelchair forward and slowly lower it down the low kerb.

Warning: When going down a low kerb, the front castors must be raised to prevent the user from falling forward. The above are only recommendations and may not be suitable for all events.



WARNING

After any adjustments, and before use, make sure all attaching hardware is tightened securely. Otherwise, injury or damage may result. As with any vehicle, the wheels and tyres should be checked periodically for cracks and wear, and should be replaced when necessary.

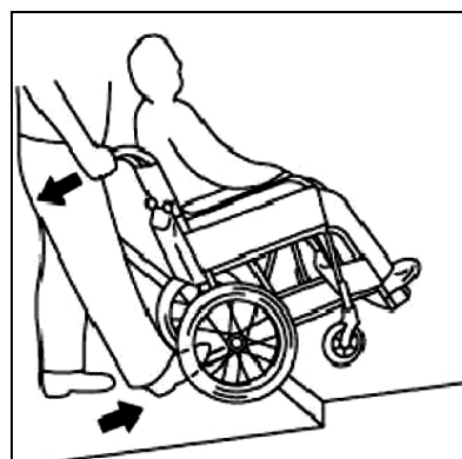

1. Evocare provides consumers with the following warranty in relation to this Product, in addition to complying with the requirements of any relevant legislation, including the *Competition and Consumer Act 2010* (Cth) in Australia and the *Consumer Guarantees Act 1993* in New Zealand (the Acts), except where a New Zealand consumer acquires the Product for the purposes of a business.

2. In this warranty, we have used the following definitions:

(a) **Form** means a warranty claim form issued by Evocare in respect of Products;

(b) **Evocare** or **our** means Evocare Australia Pty Limited, ABN 98 078 566 604 of Level 19, 144 Edward Street, Brisbane 4000;

(c) **Products** means the goods manufactured for Evocare (including products manufactured by its contract manufacturers);

(d) **Material** means a material or component used by Evocare in the manufacture of the Products;

(e) **Retailer** means the authorised dealer of Products from whom the Product was purchased;

(f) **Warranty Period** means the warranty period commencing from the date of purchase of the relevant Product. If the Product or part (as the case may be) is repaired or replaced, there will be no extension to the original warranty period; and

(g) **Workmanship** means the handling, assembly and manufacturing processes performed by or on behalf of Evocare in order to manufacture the Products.

3. Evocare warrants that for the duration of the Warranty Period, all Products will be free of faults arising from defects in Workmanship or Materials, on the terms and conditions set out in this warranty.

4. Evocare undertakes that if during the Warranty Period any Product, or any part of a Product, has failed to operate correctly due to faulty Workmanship or defective Material, it will repair or replace the Product or part (as the case may be) free of charge provided that the following procedures are met :

(a) The consumer must contact the Retailer or Evocare upon becoming aware of any defect to a Product upon which the consumer will be required to complete a Form and provide satisfactory proof of purchase.

(b) Evocare will review the Form to determine whether there is a defect, and if so Evocare agrees to (at its option) repair, replace or supply equivalent goods, or pay the cost of any of those remedies to the consumer.

(c) If Evocare requests the return of the applicable Product or part, the consumer will be responsible for the collection and freight costs of returning that Product or part to Evocare.

(d) The consumer acknowledges that it is also responsible for the freight costs to deliver any new Product or replacement part to it.

5. This warranty is in addition to any non-excludable legal rights or remedies conferred on the consumer under any applicable Act and any similar laws. To the extent permitted by law, Evocare's liability for any non-excludable condition or warranty is limited to rectifying any defect at its option, as set out in paragraph 4(b).

6. Subject to the requirements of any applicable Act or legislation and to the extent permitted by law, no liability (whether expressed or implied) of any nature whatsoever, is accepted by Evocare for any consequential loss, damage or injury arising as a result of any fault in the Products.

7. This warranty does not extend to damage to Products which occurs during transit or transportation, or which is caused by any abuse, accident or improper installation, connection, use, adjustment or repair or use of goods otherwise than in accordance with instructions issued by Evocare.

8. The warranty on Products is waived if any addition or attachment to the Products do not have Evocare's approval or are not sold as Evocare products. The Products are designed to perform specific tasks under established test loads and unauthorised attachments may produce stresses for which the design is not appropriate.

9. The following applies to consumers who purchased a relevant Product in Australia:

Our goods come with guarantees that cannot be excluded under the Australian Consumer Law. You are entitled to a replacement or refund for a major failure and compensation for any other reasonably foreseeable loss or damage. You are also entitled to have the goods repaired or replaced if the goods fail to be of acceptable quality and the failure does not amount to a major failure.

Your Evocare Mighty Bariatric Wheelchair is warranted to be free of defects in material and workmanship for 12 months, for the original consumer.

This warranty does not cover device failure due to owner misuse, negligence, or normal wear and tear.

The warranty does not extend to non-durable components such as rubber accessories, brakes and grips, which are subject to normal wear and tear. Non-durable components are warranted for 3 months.

For more information about your LM9808 Mighty Bariatric Wheelchair, warranty or to order parts call 07 3355 8007.

E- mail: sales@evocare.com.au

Website www.evocare.com.au

Manufactured for:

Evocare Australia Pty Limited, 260 South Pine Road, Enoggera. QLD. 4051.

Phone: 07 3355 8000

FAX: 07 3355 5043