
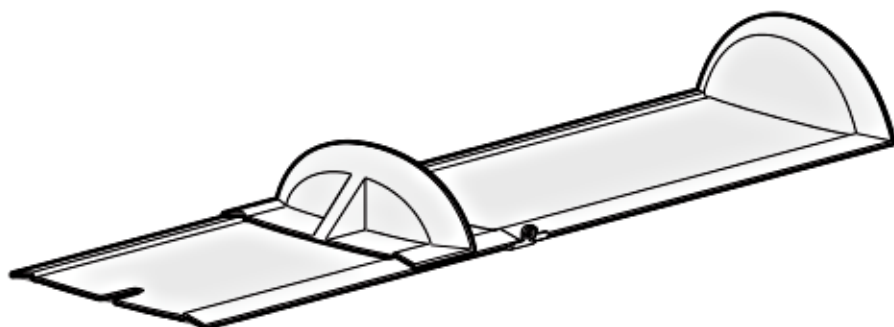


seca 417


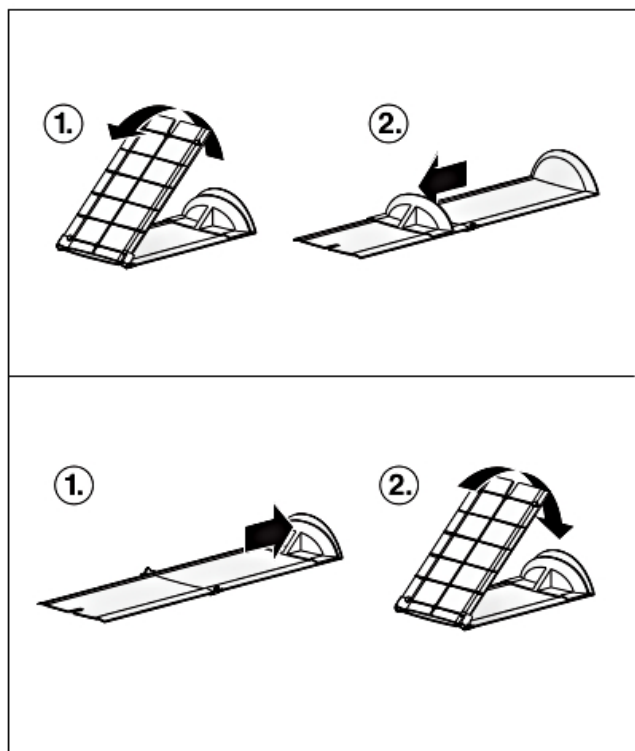


Before you start...









seca 417

Operation/Cleaning •



Technical data •

					
1 mm 1/16 inch	±5 mm	10 - 100 cm 4 - 39 inch	+10°C ... +40°C	a = 310 mm b = 1120 mm c = 120 mm	1,6 kg

seca 417

CE 0123 Declaration of conformity

The equipment for measuring length **seca 417** meets the applicable requirements of Directive 93/42/EEC (class I with measuring function) on medical products.
Batch no.: see ID plate

Hamburg, Oktober 2009



Sönke Vogel
Geschäftsführer Finanzen & Technik
seca gmbh & co. kg.
Hammer Steindamm 9-25
22089 Hamburg
Telefon: +49 40 200 000-0
Telefax: +49 40 200 000-50
i: www.seca.com

seca deutschland

Medical Scales and Measuring Systems

seca gmbh & co. kg.

Hammer Steindamm 9-25

22089 Hamburg • Germany

Phone • +49 (0)40 20 00 00 0

Fax • +49 (0)40 20 00 00 50

E-mail • info@seca.com

All contact data under www.seca.com

seca
group

seca deutschland

seca france

seca united kingdom

seca north america

seca schweiz

seca zhong guo

seca nihon

seca mexico

seca austria