

Malmet (Australia) Pty Ltd



www.evocare.com.au

Ph: 07 3355 8000 Fax: 07 3355 5043

Email: sales@evocare.com.au



Head Office & Customer Service

9-11 McKay Avenue

PO Box 373

LEETON NSW 2705

ABN 95 001 717 791

Top Loading Washer Disinfector

Unit Loading Instructions





Loading Parameters:

The Top Loading Washer Disinfector has been designed within the following parameters:


- a) Hospital utensils such as wash basins and bowls, kidney dishes, tooth mugs, suction bottles and some types of surgical instruments can be washed and disinfected during each fully automatic cycle. The unit is designed to hold six large or small wash bowls, ten mugs and/or four kidney dishes. Alternative racking will allow load variations.
- b) Holding racks are designed to ensure that the force of the water does not dislodge articles.
- c) The unit is not designed to wash plastic jugs or non-standard hospital utensils.
- d) When loading the unit it is important to ensure that sprays are positioned directly into the utensil that is being washed.
- e) It is recommended that factory supplied racks are used with the unit to ensure the most economical and efficient wash.
- f) Do not overload the unit as wash efficiency is reduced.



Head Office & Customer Service
9-11 McKay Avenue
PO Box 373
LEETON NSW 2705


ABN 95 001 717 791

Unit Loading Diagram:

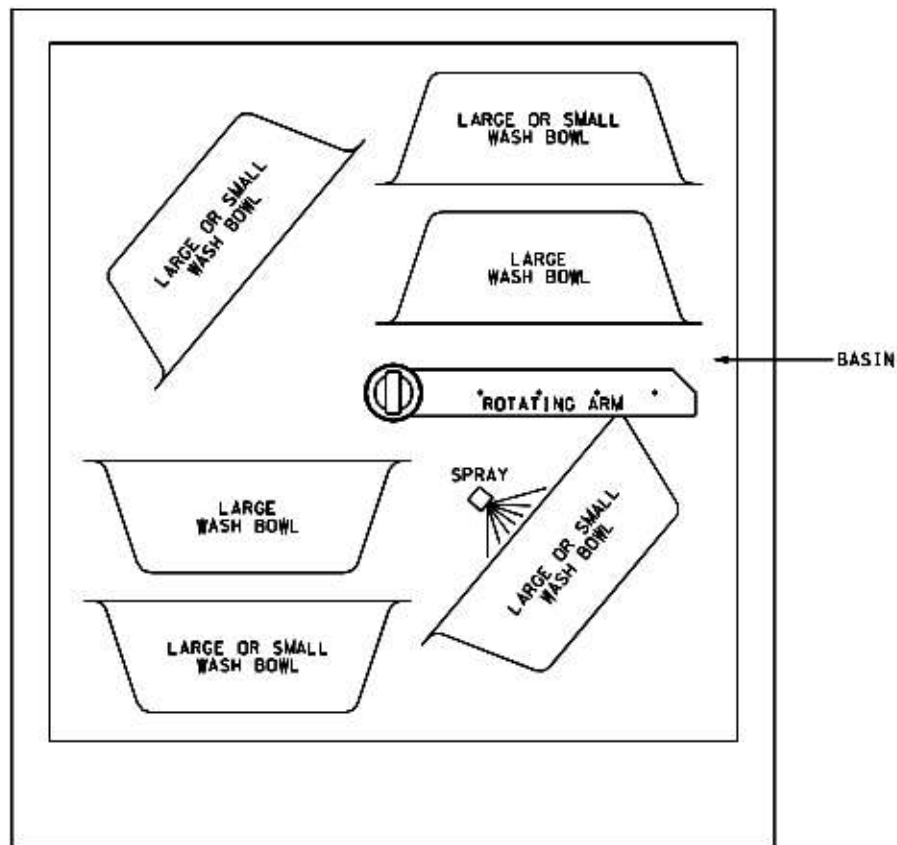

FRONT OF MACHINE

LOADING DIAGRAM - VIEW LOOKING DOWN INTO BASIN

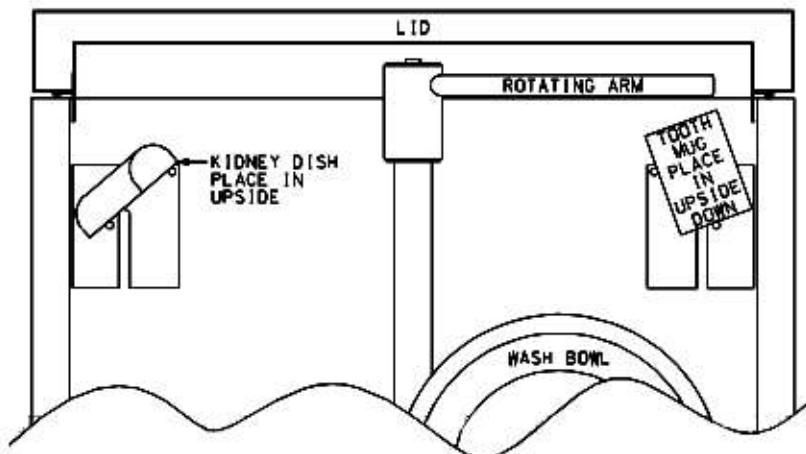



Top view of unit:



Racks to hold
tooth mugs and
some small
kidney bowls

Rack for larger bowls

Small Rack to be
inserted for smaller
bowls and larger
kidney dishes



Head Office & Customer Service
9-11 McKay Avenue
PO Box 373
LEETON NSW 2705


ABN 95 001 717 791

Standard Holding Racks:

Small Rack 8-M00-81-118



Main Rack 8-M00-81-117

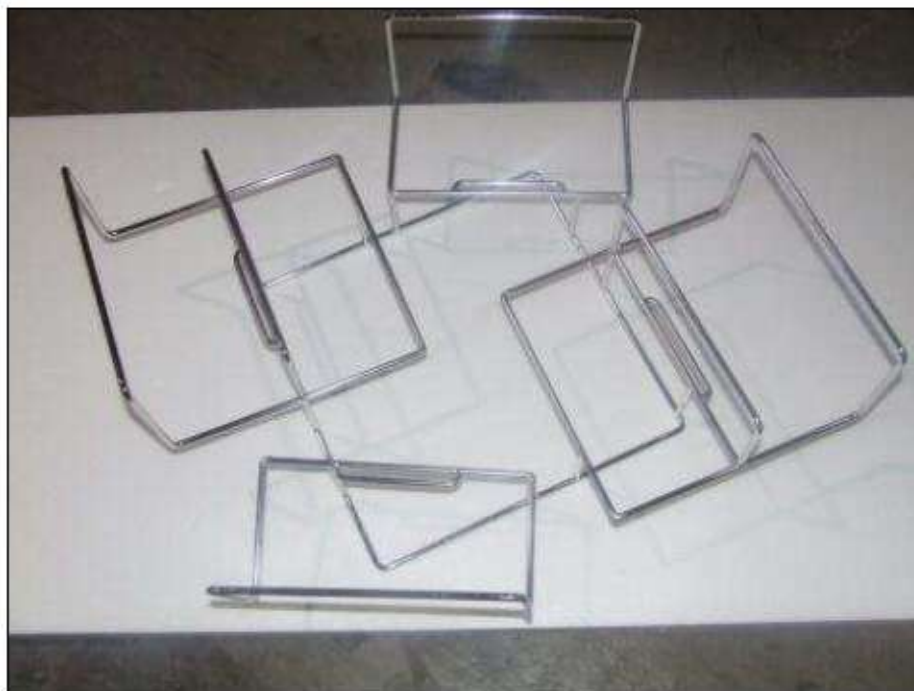



Cup Rack 8-M00-81-215



Non-Standard Holding Racks: (Can be purchased separately)

Instrument Basket Assembly 8-M00-81-116





Non-Standard Holding Racks: (Can be purchased separately)

Rectangle Tray Rack Assembly
Part No – 8-K00-81-070



Rectangle Tray Rack Assembly:





Example 1

Unit fully loaded using the Cup Rack on either side of unit.



Tooth mugs, must be face down

Large bowl, positioned without bowl rack insert.

Small bowl, positioned using bowl rack insert.

Small kidney bowls only, must be face down to ensure effective wash.



Example 2:

Unit fully loaded using instrument basket on one side and a cup rack on the other side



Instrument basket - Can also be used for scissors and knives, must be face down,

Cup Rack - Small kidney bowls only or tooth mugs, must be face down to ensure effective wash.



Example 3:

Bowls must be loaded upright, within racks provided and spray nozzles pointing directly into the bowl



Bowls loaded upright within racks provided

Spray Nozzle pointing directly into bowl



Head Office & Customer Service
9-11 McKay Avenue
PO Box 373
LEETON NSW 2705

ABN 95 001 717 791



Small bowl
positioned
using small
rack insert

Spray nozzle to
point directly into
bowl



Loading Detergent Bottles:

1. Open Detergent Holder Door



2. Remove empty detergent bottle, unscrew the lid and remove the tube.



3. Remove the lid from new detergent bottle



4. Fit bottle cap with tube attached to the full detergent bottle



5. Insert full detergent bottle into detergent holder with cap to outside



6. Push the tube to the bottom of the detergent bottle
7. Close the detergent holder door.

